



Product catalog 2022

IMPLADENT®

A decorative graphic at the bottom of the page consisting of several overlapping, wavy, translucent blue lines that create a sense of movement and depth.

Dear business partners,


The production of **IMPLADENT** implants and surgical instruments has been discontinued. We are only selling our existing stock. The core range of **IMPLADENT** prosthetic and laboratory components, together with the compatible instruments is, however, still available for the 2.9, 3.7 and 5.0 prosthetic series.

Implants overview	5
Gingiva formers	6
STANDARD abutments for cemented restorations	7
PLUS abutments for cemented restorations	8
Abutments for screw-retained restorations	9
Individual prosthetic solutions	10
LOCATOR attachments	11
Ball attachments	12
Impression and laboratory components	13
Components for D5.0-C implants	14
Instruments	15
Additional components	17
ProImplant	18
Terms and conditions	19

IMPLADENT Implant System

MEDICAL MANUFACTURER WITH A LONG TRADITION

Since 1991, LASAK, as a research-oriented medical technology company, has been focusing on the systematic research and development of bone regeneration materials and implants used in dental implantology, neurosurgery, orthopaedics and traumatology. The results of research and development, as well as the success rate in clinical practice, are systematically evaluated, used in product innovation and published in prestigious journals. LASAK offers its clients modern, safe and clinical verified solutions at the highest technological level.

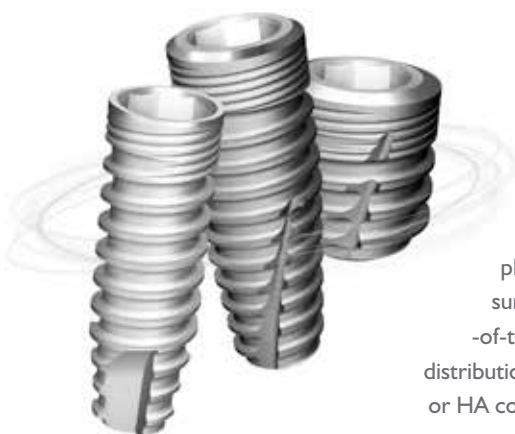

IMPLANT SYSTEM

The IMPLADENT implant system includes ACCEL – tapered implants offering easy insertion and high primary stability in soft bone as well as straight implants for easy positioning in dense bone. The horizontal and vertical set-off of the implant-abutment connection from the bone level together with the implant mini-threads, contribute to the stability of the marginal bone and soft tissues surrounding the abutment and provide improved restoration aesthetics. The state-of-the-art implant construction enables safe and precise insertion and optimized load distribution in the bone tissue. Implants are available with a unique bioactive, sand-blasted or HA coated surface. A single system organizer provides instruments for the insertion of implants with both tapered and straight design.


QUALITY MANAGEMENT SYSTEM

LASAK manufactures and markets medical devices of all classes, even those for the IIb and III risk classes. Production takes place in clean areas that are validated on an annual basis and fulfill the strict requirements of the EN ISO 14644 standard. LASAK complies with all requirements imposed by legislation as well as the requirements of its quality management system in compliance with the EN ISO 13485 standard and is a holder of QMS certificates (confirming that the management system guarantees quality).

All LASAK products bear the CE mark.


WHY IMPLADENT FROM LASAK?

- Long-term scientific documentation
- Unique hydrophilic bioactive nanostructured titanium surface
- Exceptionally universal application
- Option of reduced treatment time – safe early and immediate loading
- Tapered and straight implants for both soft and dense bone in one organizer
- One universal prosthetic platform yielding maximum flexibility
- Wide range of prosthetic components ensuring perfect esthetic results
- Cost-effective temporary treatment

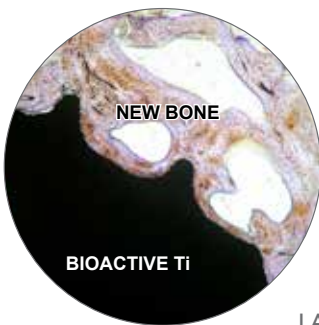

BIO – THE FIRST NANOSTRUCTURED, HYDROPHILIC, BIOACTIVE SURFACE

As a result of long-term, continuous research into biomaterial – body environment interactions, the IMPLADENT system is the first implant system on the market that is able to offer unique nano-structured, hydrophilic and bioactive surface treatment. The invention of the BIO-surface has given LASAK a leading global position in the development of implant surface modifications. LASAK's unique BIO-surface modification speeds up the formation of a functional boneimplant interface, thus improving the implant's secondary stability in the early healing phase. Thanks to the BIO-surface, the stability dip, often observed in nonbioactive surfaces, is eliminated. The outstanding performance of BIO-surface implants has been documented for even the most demanding indications.

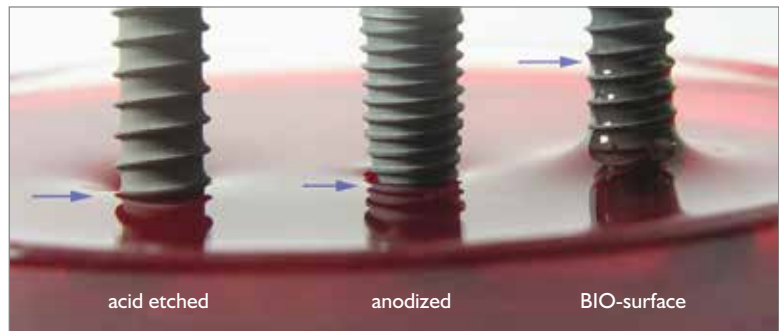

SCIENTIFIC DOCUMENTATION


We will be glad to send you a 80-page summary of selected clinical and experimental studies documenting the long-term clinical performance and scientific background of LASAK products.



The IMPLADENT implants have been discontinued and can no longer be ordered. This page provides an overview for their easier identification.

IMPLANTS – STRAIGHT

Implants – series 2.9



D2.9 SB



● Prosthetic platform 2.9

Implants – series 3.7




D3.7 BIO D3.7 STIO C2.5 D3.7 VHAO



● Prosthetic platform 3.7

Implants – series 5.1




D5.1 BIO




● Prosthetic platform 3.7

Implants – series 5.0



D5.0 STI-BIO-C D5.0 VHAO



● Prosthetic platform 5.0

Prosthetic platforms



Red prosthetic platform 2.9 is intended for narrow D2.9 IMPLADENT implants.

Green prosthetic platform 3.7 is intended for D3.7, D4.4, D5.1 and D5.6 IMPLADENT implants.

Blue prosthetic platform 5.0 is intended for D5.0 IMPLADENT implants.

The matching of the prosthetic and laboratory components to the corresponding prosthetic platform is indicated in the catalog by colored symbols.

- platform 2.9
- platform 3.7
- platform 5.0

IMPLANTS ACCEL – TAPERED

Implants – series 4.4




D4.4 BIO-ACCEL D4.4 HA-ACCEL



● Prosthetic platform 3.7

Implants – series 5.6



D5.6 BIO-ACCEL D5.6 HA-ACCEL



● Prosthetic platform 3.7

STI – Threaded implants without octagon
 VHAO – Cylindrical implants with internal octagon
 VHA – Cylindrical implants without octagon
 STIO/SHAO/STI-BIO-C – Threaded implants with internal octagon


The D3.7 and D3.6 implants manufactured before 1996 do not have an internal octagon, therefore, the prosthetic components for them must be manufactured as a custom-made medical device.

The illustrations do not represent products in their actual sizes.



Gingiva formers


Extra strong abutment screw M2.3^{con}

The abutment screw of the green prosthetic platform 3.7 is, with its diameter of 2.3 mm, at least 30 % stronger than conventional screws M2.0. The stronger screw gives extra strength to the implant-abutment connection and allows a high tightening torque. This minimizes the risk of any eventual gap from lateral loading, especially when used with implants of a wider diameter. The stronger screw gives extra stability to the linear anchored restorations and to other restorations supported by non-optimally placed implants. The cone under the screw head provides reliable, tight locking of the screw and prevents its eventual loosening.





Gingiva formers – narrow

			
		L2	L4
D3.7/d4.0 narrow	●	222.3	422.3
D2.9/d3.9 narrow	●	1022.3	1222.3



Gingiva formers esthetic – wide

			
		L2	L4
D3.7/d5.2 wide	●	622.3	822.3
D2.9/d4.7 wide *	●	3122.3	3322.3

* Available within three weeks from the order date.

Throughout the catalog the abbreviations D and d are used as follows:


D – relates to the prosthetic series diameter (green platform 3.7, red platform 2.9, blue platform 5.0)

d – relates to the actual diameter in specific cases

The gingiva former should extend over the edge of the adapted soft tissue by 1.0 to 2.0 mm, thus preventing the gingiva former becoming covered by edematous tissue during the post-operative period. The gingiva former's diameter must match the diameter of the abutment to be used in the prosthetic work.

STANDARD abutments for cemented restorations

- Allows chair-side selection of the best suitable abutment
- Easy and straightforward impression
- Wide choice of cuff (L) and angulations




STANDARD abutments for cemented restorations – straight



	L1	L2	L3	L4
D3.7/d4.8 wide	● 1132.3	2132.3	3132.3	4132.3

Spare abutment screw for abutment D3.7/d4.8 may be ordered separately under Ref. No. 552.3.




STANDARD abutments for cemented restorations – straight



	L1	L2	L3	L4
D3.7/d3.7 without octagon wide *	● 112.3	212.3	312.3	412.3
D3.7/d4.8 without octagon wide *	● 10122.3	20122.3	30122.3	40122.3
D2.9/d3.7 without octagon narrow *	● 152.3	252.3	352.3	452.3

* Available within three weeks from the order date.



STANDARD abutments for cemented restorations – angulated



	L1	L2	L3	L4
D3.7/d4.8/15° wide *	● 1142.3	2142.3	3142.3	4142.3
D3.7/d4.8/25° wide *	● 1152.3	2152.3	3152.3	4152.3
D2.9/d3.7/15° narrow *	● 1102.3	2102.3	3102.3	4102.3
D2.9/d3.7/25° narrow *	● 1112.3	2112.3	3112.3	4112.3

Spare abutment screws may be ordered separately under Ref. No. 552.3 for green platform abutments and Ref. No. 752.3 for red platform abutments.

* Available within three weeks from the order date.

IMPRESSION – implant level

see page 13

Open tray impression post	Implant analog
D3.7/d4.8 narrow ● 533.3	D3.7 with retention ● 513.3
D2.9/d3.7 narrow ● 933.3	D2.9 with retention ● 813.3


Abutment not suitable for single tooth restoration.

Use a new abutment screw for the final abutment tightening.
Tightening torque of abutment screw is 35 Ncm.




Esthetic PLUS abutments for cemented restorations

- Emergence profile similar to natural tooth Extra robust design
- Easily scanable

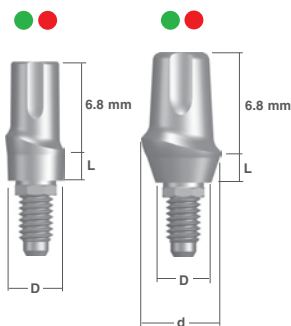The re-designed LASAK Esthetic PLUS abutment is an universal supraconstruction generally usable for almost all kinds of cement retained restorations. It gives the technician more flexibility when shaping the abutments according to individual requirements. The shape of the abutment predetermines it for use when restoring frontal teeth. The extra robust design of the abutment gives superior stability and offers extra surface for the bond when used posteriorly. The oval shape resembles the emergence profile of a natural tooth. The curve of the abutment shoulder allows for easy scanning by almost all kinds of dental scanning systems, and for easy wax-up. Double guide slots ensure perfect positioning of the crown when cemented.




Esthetic PLUS abutments for cemented restorations – straight




				
		L1	L2	L4
D3.7/d4.0 narrow *	●	15252	25252	45252
D3.7/d5.4 wide *	●	515252		
D2.9/d3.8 narrow *	●	1121.01	1121.02	
D2.9/d4.4 wide *	●	615252	625252	

Spare abutment screws may be ordered separately under Ref. No. 552.3 for green platform abutments and Ref. No. 752.3 for red platform abutments.

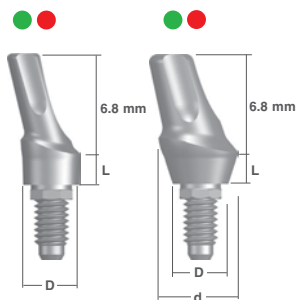* Available within three weeks from the order date.



Esthetic PLUS abutments for cemented restorations – angled

				
		L1	L2	L4
D3.7/d4.0/15° narrow *	●	15192	25192	45192
D3.7/d4.0/25° narrow *	●	15202		
D3.7/d5.4/15° wide *	●	515192	525192	545192
D3.7/d5.4/25° wide *	●	515202		
D2.9/d3.8/15° narrow *	●	1122.01	1122.02	
D2.9/d4.4/15° wide *	●	615192	625192	
D2.9/d4.4/25° wide *	●	615202		

Spare abutment screws may be ordered separately under Ref. No. 552.3 for green platform abutments and Ref. No. 752.3 for red platform abutments.

* Available within three weeks from the order date.

IMPRESSION – implant level


see page 13

Open tray impression post		Implant analog	
D3.7/d4.8 wide	● 533.3	D3.7 with retention	● 513.3
D2.9/d3.7 wide	● 1233.3	D2.9 with retention	● 813.3







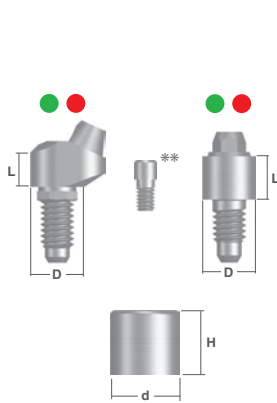

Use a new abutment screw for the final abutment tightening.
Tightening torque of abutment screw is 35 Ncm.

Abutments for screw-retained restorations

- Easily revisible restoration
- Both occlusal and transversal fixation possible






Abutments for screw-retained restorations

		 L1	 L2	 L3	 L4
D3.7/d3.7 narrow *		10042.3	11042.3	12042.3	13042.3
D2.9/d3.7 narrow *		30042.3	31042.3	32042.3	33042.3
D3.7/25° angulated *			230202	240202	250202
D2.9/25° angulated *			130202	140202	150202
Healing cap for abutments for screw-ret. rest. D3.7/d4.8/H4.5 *					2333.3





** Spare bridge screws may be ordered separately under Ref. No. 1641.3. Spare abutment screws may be ordered separately under Ref. No. 552.3 for green platform abutments and Ref. No. 752.3 for red platform abutments.
* Available within three weeks from the order date.

IMPRESSION – abutment level

		see page 13	
Impression coping		Abutment analog	
D3.7 (D2.9)/H8 narrow	 	D3.7 (D2.9)/H8 narrow	 
	12033.3		7013.3

Transversal screws



L1 *		146.3
L2		246.3
L3		346.3
L4 *		446.3

The head length (L) of the transversal screw should be chosen according to the anatomy of the crown.
* Available within three weeks from the order date.

 Abutment not suitable for single tooth restoration.

Tightening torque of abutment screw is 35 Ncm.
Tightening torque of bridge and transversal screw is 15 Ncm.

Individual prosthetic solutions

LASAK CadCam bridges and abutments

LASAK CadCam technology represents a unique production system of precise superstructures which allows direct fixation in dental implants without the use of abutments or other connecting elements. This reduces the number of gaps, between the implant and the superstructure, which can be a potential source of bacterial contamination. LASAK CadCam bridges and abutments are available for these implant systems: LASAK Impladent and BioniQ, Astra Tech®, NobelActive™, NobelReplace®, Straumann® Bone Level and SynOcta®.



LASAK CadCam bridges

	Pontic (price/unit)	Implant-supported unit (price/unit)
Ti, Co-Cr	D01	D02
ZrO ₂ *	D07	D08
SCAN/CAD		D10

* The ZrO₂ superstructures are delivered with Ti bases.

The price of the superstructure includes the fixing screws for connecting to the implant. The price applies when STL data has been supplied.



LASAK CadCam custom abutments

Ti/Co-Cr	D03
ZrO ₂ *	D04
SCAN/CAD	D10

* It is delivered with Ti abutment.

Custom abutments always contain compatible screws. The price is by delivering STL data.



LASAK CadCam abutments for LASAK Impladent (Ti base)

IMPLADENT D3.7, without octagon	●	1107.00
IMPLADENT D3.7, with octagon *	●	1128.00
IMPLADENT D2.9, without octagon *	●	1108.00
IMPLADENT D2.9, with octagon *	●	1131.00

* Available within three weeks from the order date.



Scanbodies

IMPLADENT D3.7, with octagon	●	1801.00
IMPLADENT D2.9, with octagon	●	1802.00



Cast-On abutment for LASAK Impladent

IMPLADENT D3.7, with octagon *	●	1161.00
--------------------------------	---	---------

* Available within three weeks from the order date.

The small LASAK CadCam bridges are delivered within 3–5 working days and the large LASAK CadCam bridges are delivered within 5–7 working days. For more information ask for the LASAK CadCam leaflet and price list.

- Dual retention
- Self-aligning feature
- Minimal vertical height



The diameter of the LOCATOR attachment is 3.85 mm. In the case of even minimal override of marginal bone to the implant platform make sure to remove it. 1.5 mm of the bronze-colored LOCATOR part should remain supragingival to be able to retain the over-denture.

LOCATOR attachments		L0	L1	L2	L3	L4	L5
D3.7	●	01207	01208	01209	01210	01211	01212



LOCATOR processing package

LOCATOR processing package (denture cap, black processing insert, set of retentive inserts, block-out spacer), 2 pcs. of each type 08519-2



LOCATOR replacement inserts

Blue 680 g, set of 4 pcs.	08529
Pink 1,361 g, set of 4 pcs.	08527
Clear 2,268 g, set of 4 pcs.	08524
Red 680 g, extended range, set of 4 pcs.	08548
Orange 907 g, extended range, set of 4 pcs.	08915
Green 1,814 g, extended range, set of 4 pcs.	08547

For implant disparallelity over 10° (max. 20°) use an extended range insert.



Instruments



LOCATOR driver for IMPLADENT ratchet	09999
LOCATOR driver	08913
LOCATOR core tool	08393




IMPRESSION and laboratory components

LOCATOR impression coping	LOCATOR abutment analog
4 pcs. 08505	4 pcs. 08530

Tightening torque of attachment is 35 Ncm.

Ball attachments

- Long established, reliable and cost-effective solution
- Optimum combination – titanium/gold
- Retention strength repeatedly adjustable



Ball attachments CLASSIC		L1	L2	L3	L4	L6
D3.7/d3.7	●	21432:3	22432:3	23432:3	24432:3	26432:3
D2.9/d3.7	●	55432:3	56432:3*	57432:3*	58432:3*	60432:3*

* Available within three weeks from the order date.



Retentive cap CLASSIC

Matrice CLASSIC	6932.3
Matrice CLASSIC eliptická	7932.3



Retentive cap CLASSIC Plus

Retentive cap CLASSIC Plus	055752
Retentive cap CLASSIC Plus elliptic	055890



Starter set CLASSIC

Starter set CLASSIC 2 * (ball attachments 2x, retentive cap 2x, space maintainer 2x, activator, deactivator)	13932.3
Starter set CLASSIC 6 * (ball attachments 6x, retentive cap 6x, space maintainer 6x, activator, deactivator)	14932.3

* Available within three weeks from the order date.



Instruments

Activator for retentive cap CLASSIC	8932.3
Deactivator for retentive cap CLASSIC	9932.3



Retentive cap driver CLASSIC Plus	072609
-----------------------------------	--------



Protective ring fitting tool CLASSIC	10932.3
--------------------------------------	---------



Insertion wrench, short L5 *	2024.3
Insertion wrench, long L13 *	324.3




Space maintainer for ball attachment CLASSIC *	● ● 543:3
--	-----------

* Available within three weeks from the order date.

When using ball attachments, the height of the cuff (L) should be level with, or 1.0 mm above, the gingiva. Sufficient space should always be left to enable the retentive cap to be affixed using the self-curing base resin and to retain the necessary mechanical resistance of the basal resin during the occlusal loading of the hybrid restorations.

Tightening torque of attachment is 35 Ncm.



Open tray impression posts (fastening pin included)

D3.7/d3.7 narrow	●	633.3
D3.7/d4.8 wide	●	533.3
D2.9/d3.7 narrow	●	933.3
D2.9/d4.5 wide	●	1233.3



Impression coping for screw-retained restorations (fastening pin included)

D3.7/d4.8/H8	●	12033.3
--------------	---	---------



Implant analogs

with retention D3.7	●	513.3
with retention D3.7 3D print **	●	1830.00
without retention D3.7 *	●	913.3
with retention D2.9	●	813.3
with retention D2.9 3D print **	●	1829.00

Spare abutment screws may be ordered separately under Ref. No. 552.3 for green platform abutments and Ref. No. 752.3 for red platform abutments.

* Available within three weeks from the order date.

** Available from May 2022.



Abutment analog for screw-retained restorations

with retention D3.7 (D2.9) narrow	● ●	7013.3
-----------------------------------	-----	--------

Spare bridge screws may be ordered separately under Ref. No. 1641.3.



Burn-out coping for cemented restorations – STANDARD abutments

with shoulder D3.7 (D2.9) narrow	● ●	453.3
without shoulder D3.7 (D2.9) narrow *	● ●	253.3
with shoulder D3.7/d4.8 wide	●	553.3
without shoulder D3.7/d4.8 wide	●	353.3


* Available within three weeks from the order date.



Burn-out coping for screw-retained restorations

D3.7 (D2.9)	● ●	1153.3
-------------	-----	--------

Components for D5.0-C implants

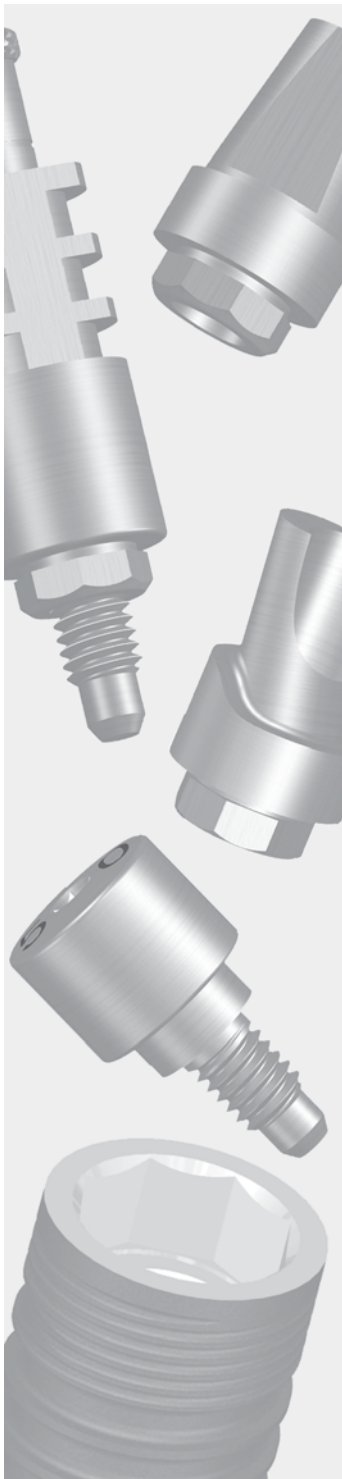

Gingiva formers

		L2	L4	L6
D5.0 straight	●	2122.3	2322.3	4022.3

STANDARD abutments for cemented restorations

		L1	L2	L3	L4
D5.0 straight	●	125.3	225.3	325.3	425.3
D5.0/15°	●	135.3	235.3	335.3	435.3
D5.0/25°	●	145.3	245.3	345.3	445.3

Abutments for screw-retained restorations

		L1	L2	L3	L4
D5.0	●	155.3	255.3	355.3	455.3
Insertion tool for abutments for screw-retained rest. L10/L22					4524.3

Ball attachments – CLASSIC

		L1	L2	L3	L4
D5.0	●	41432:3	42432:3	43432:3	44432:3

Temporary abutment

		L1
D5.0	●	2055.3

Impression components

Open tray impression post		●	1123.3
Impression abutment coping STANDARD		●	1133.3
Impression coping for screw-retained restorations		●	2133.3

Laboratory components

Implant analog with retention		●	1173.3
Abutment analog for screw-retained rest. with retention		●	1143.3
Burn-out coping STANDARD with shoulder		●	653.3
Burn-out coping for screw-retained restorations		●	2253.3

Spare abutment screw for prosthetic platform D5.0 may be ordered separately under Ref. No. 652.3. Components for D5.0-C implants are available within three weeks from the order date.

Ratchet


The ergonomic IMPLADENT ratchet with its torque adapter is designed for surgical as well as prosthetic application. It is manufactured from high-strength, corrosion-resistant stainless steel and withstands the most demanding working conditions. The easy-change reversible mechanism ensures a comfortable change of the working motion without the need to dismount the ratchet from the site.



Ratchet

Ratchet	2409.00
---------	---------

Screwdrivers for ratchet




extra short, hex 1.4/L4	24224.3
short, hex 1.4/L11	4224.3
long, hex 1.4/L21	4024.3
for screw-retained restorations short, hex 1.0/L11	44224.3
for screw-retained restorations long, hex 1.0/L21	24024.3

Screwdriver mechanical



Hex screwdriver mechanical hex 1.4	8224.3
------------------------------------	--------


Implant insertion wrench – Extension wrench



Implant insertion wrench, short L5/L17 *	2024.3
Implant insertion wrench, long L13/L25	324.3
Extend driver	4214.3


* Available within three weeks from the order date.

Hex hand screwdrivers intraoral



extra short hex 1.4/L11/L18	3224.3
short hex 1.4/L11/L25	2224.3
long hex 1.4/L21/L35	2524.3
for screw-retained restorations short, hex 1.0/L11/L25	5224.3
for screw-retained restorations long, hex 1.0/L21/L35	6224.3

Insertion tool for abutments of screw-retained restorations



short D3.7 (D2.9)/L5/L17 *	7113.3
long D3.7 (D2.9)/L10/L22 *	70113.3

* Available within three weeks from the order date.

Explantation wrench





Explantation wrench L10/L22	4524.3
-----------------------------	--------

Guide to screwdrivers and tightening torques

Screwdrivers

The IMPLADENT implant system features two main groups of fixing screws – the abutment screws and the bridge screws. For tightening of the abutment screws (as well as implant cover screws, gingiva formers and other components) use IMPLADENT screwdriver **hex 1.4**. To handle bridge screws which fit to Abutments for screw retained restorations use IMPLADENT screwdriver **hex 1.0**.



Hex hand screwdrivers intraoral

hex 1.4 /L11/L18, extra short	3224.3
hex 1.4 /L11/L25, short	2224.3
hex 1.4 /L21/L35, long	2524.3
for screw-retained restorations hex 1.0 /L11/L25, short	5224.3
for screw-retained restorations hex 1.0 /L21/L35, long	6224.3

Screwdriver mechanical



Hex screwdriver mechanical hex 1.4	8224.3
---	--------


To make sure the implant-abutment interface is really tight and to avoid loosening of a crown make sure to tight the abutment screw with help of Ratchet. Tightening torque of abutment screws is generally 35 Ncm. Use new abutment screw for final placement of the abutment. For tightening of bridge screws and some other special components different tightening torques apply – please see below.



Ratchet

Ratchet	2409.00
---------	---------

Screwdrivers for ratchet



hex 1.4 /L4, extra short	24224.3
hex 1.4 /L11, short	4224.3
hex 1.4 /L21, long	4024.3
for screw-retained restorations hex 1.0 /L11, short	44224.3
for screw-retained restorations hex 1.0 /L21, long	24024.3

Tightening torque overview

Abutment screws / Screwdrivers **hex 1.4** (24224.3, 4224.3, 4024.3) / tightening torque 35 Ncm
 Temporary abutments PEEK / Screwdrivers **hex 1.4** (24224.3, 4224.3, 4024.3) / tightening torque 20 Ncm
 Bridge screws / Screwdrivers **hex 1.0** (44224.3, 24024.3) / tightening torque 15 Ncm
 Ball attachments / Extension wrench (2024.3) / tightening torque 35 Ncm
 Locators / Locator driver / tightening torque 35 Ncm
 Titanmagnetics abutment / Dedicated drivers (H.00.04.X2, H.00.04.K2) / tightening torque 20 Ncm

There is a set of prosthetic instruments, please see ref 834.3, containing ratchet and **hex 1.4** and **hex 1.0** screwdrivers available for loan. The minimum rental period is 14 calendar days (including the date of delivery to the customer and the date of return to the LASAK company). The goods can be rented for a maximum of 28 days. Prior to returning the goods, it is necessary to ensure that they are functional, dry, and free of all dirt. If the rented goods are not returned in accordance with the above conditions, or if the goods are returned damaged, the full price of the goods will be charged.

Use new abutment or bridge screw for placement of the final prostheses.

Additional components for the IMPLADENT system



Prosthetic set

Prosthetic set IMPLADENT	834.3
Prosthetic set for cemented restorations	734.3



Prosthetic set IMPLADENT contains: Ratchet with torque adapter*, Extension wrench*, Insertion tools for abutments of screw-retained prostheses – short and long, Hex hand screwdrivers hex 1.4* and hex 1.0 – short, long, Screwdrivers for ratchet hex 1.4* and hex 1.0 – short and long. *Items included in prosthetic set for cemented prostheses.



Explantation drill

D2.9	1000.3
D3.7	1010.3
D5.1	1020.3

Use reverse motion.



Broken screw remover sets



Screw remover set IMPLADENT, D2.9 (threadformer, reverse drill, drill guide, claw drill and organizer)	1903.00
Threadformer, D2.9	2909.01
Reverse drill, D2.9	2909.02
Drill guide, D2.9	1903.03
Claw drill, D2.9	2909.04
Screw remover set IMPLADENT, D3.7 (threadformer, reverse drill, drill guide, claw drill and organizer)	1904.00
Threadformer, D3.7	1904.01
Reverse drill, D3.7	2909.02
Drill guide, D3.7	1904.03
Claw drill, D3.7	1904.04

Instructions for the removal of a damaged screw are available at www.lasak.com.

Prolimplant

- Immediate provisional restoration
- Easy and straightforward insertion
- Possibility of parallelism correction

The LASAK Prolimplant system enables esthetically demanding patients to be provided with a fixed restoration during the healing phase of permanent implants or graft sites. The installation procedure is straightforward and simple using an insertion wrench (manual or mechanical) and dedicated bending tool. After six months at the latest, or as soon as the permanent implants are restored, the Prolimplants can easily be removed using the same instruments. The accessories such as insertion wrench, impression or laboratory components are fully compatible with the IMPLADENT system.

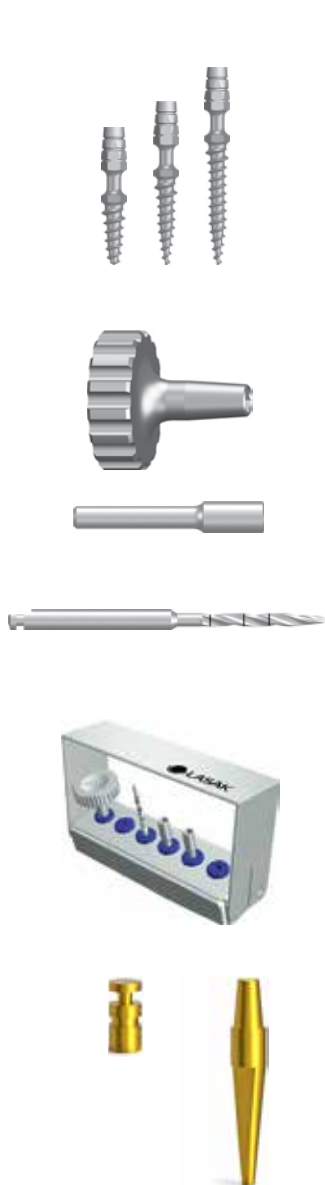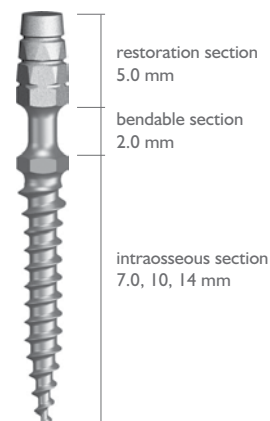

Prolimplant – implants

D2.1	L7	L10	L14
	5102.3	6102.3	7102.3
Insertion wrench			2344.3
Parallelizer			1324.3
Prolimplant – final drill, d1.5			01314.3
Surgical kit – Prolimplant (insertion wrench, parallelizer – 2 pcs., drill)			1134.3

Impression and laboratory components

Closed tray impression coping, D3.7 (D2.9)	● ●	133.3
Abutment analog, without retention, D3.7 (D2.9) – narrow	● ●	313.3

IMPLADENT GUARANTEE TERMS AND CONDITIONS

LASAK Ltd. offers a ten-year guarantee on all IMPLADENT system implants introduced after January 1, 2003. In case of implant loss or failure within ten years of the implantation date, LASAK Ltd. will replace the implant, including cover screw, free of charge, on condition that: the implant was inserted with the use of original IMPLADENT system components, and in accordance with the manufacturer's recommendations, instructions and manuals.

Entitlement to guarantee:

Claims on the guarantee will be honoured providing original surgical and prosthetic components of the IMPLADENT system were used and the implantation performed in accordance with commonly accepted medical practice and adhering to the manufacturer's instructions and recommendations as published in manuals and leaflets of LASAK Ltd. Implantations with contraindications as described in the instructions and manuals of LASAK Ltd. are not covered by the guarantee. The guarantee can be claimed solely by the medical entity that undertook the implantation, it cannot be claimed by the patient nor by any other persons. Any medical entity that is financially in debt to LASAK Ltd.

for delivered goods or services is excluded from this guarantee.

Exclusions:

This guarantee does not cover implants that are lost:

- due to a patient's insufficient oral hygiene and/or due to infections,
- as a result of a personal accident or a patient's inappropriate behaviour,
- due to overloading.

This guarantee does not cover any provisional implants.

Changes to and termination of this guarantee:

LASAK Ltd. reserves the right to make changes to or to terminate this guarantee, without prior notice.

How to make a claim under this guarantee:

To make a claim under this guarantee, a completed form 'Record of Failed Implant' should be sent, along with the sterilised implant and other components used, to the business address of LASAK Ltd. within 30 days of the implant failure.

The conditions given above are general and may vary slightly in different countries. The valid conditions of the guarantee for a given country will be provided by the representative of LASAK Ltd. in each country.

LASAK Ltd. maintains the right to modify, terminate, change specifications or prices without prior notice.

GENERAL BUSINESS TERMS

PRICING – All the above prices are ex-works (EXW) Prague, Czech Republic, Incoterms 2000 and do not include any commission, VAT or other duties nor transport or packing costs. The seller reserves the right to change the prices without prior notice.

ORDERING – Orders may be received by writing, Internet, telephone or fax. An order is deemed accepted upon confirmation by the seller or upon delivery of the products, whichever is earlier. In every order must be clearly stated the full statutory name of the buyer, delivery address, specification required, delivery date, preferred mode of transportation and contact person with their phone number.

DELIVERY TIME – The delivery time depends upon the ordered quantity and has

to be agreed individually in advance. Generally, orders are dispatched by the first available carrier within three days after receipt of the order or payment.

PACKAGING – Implants are supplied in sterile packing. Other components of the implant system are not supplied sterile, but decontaminated in sealed transparent flat bags.

PAYMENT TERMS – All listed prices are net at the account of the seller. Payment terms are payment in advance or confirmed, irrevocable, documentary L/C. If payment is late the maximum statutory interest rate will be applied to the late amount. Further deliveries may be suspended until full payment for any previous unpaid shipment has been received. All products remain in the ownership of the

seller until the full invoiced price is settled.

VALIDITY – The price list is valid from May 15, 2020.

TRANSPORTATION – An individually agreed mode of transportation is used, usually standard mail to the specified address of the customer. The transportation costs are charged separately and are not included in the listed prices.

DELIVERY TERMS AND INSURANCE

The listed prices are ex-works (EXW) Prague, Czech Republic, Incoterms 2000 delivery terms. We are prepared to ship the requested material to the specified address based on DDU, CIP or other agreed delivery terms upon request. All costs incurred are charged over and above the list price for the goods.

